

Fig. 1





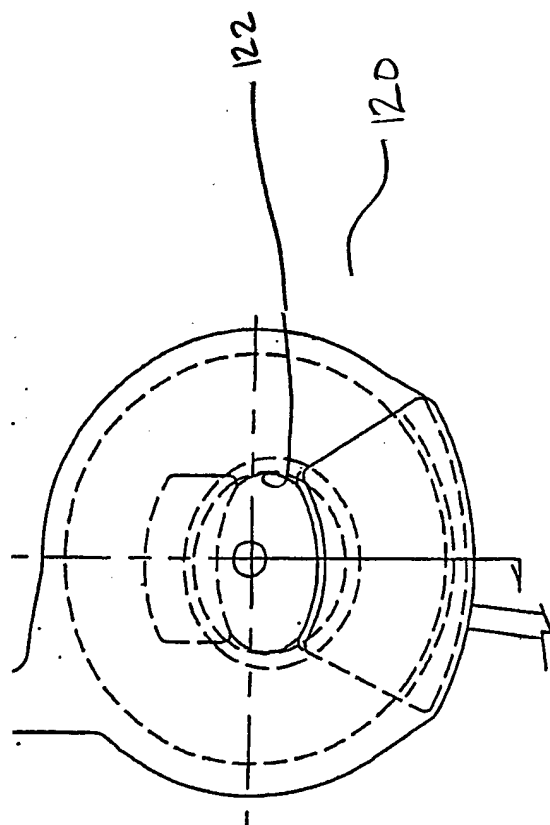



FIG. 2

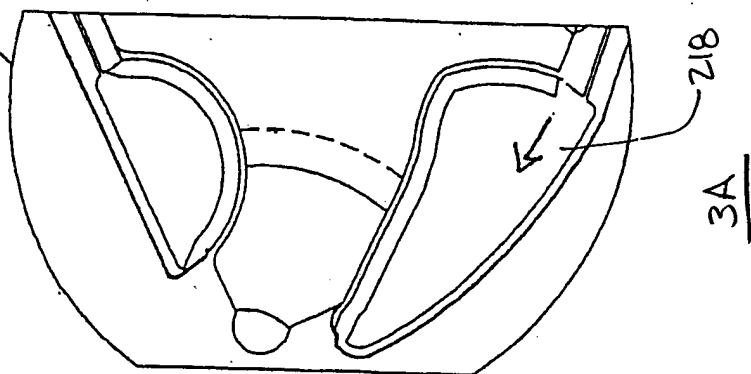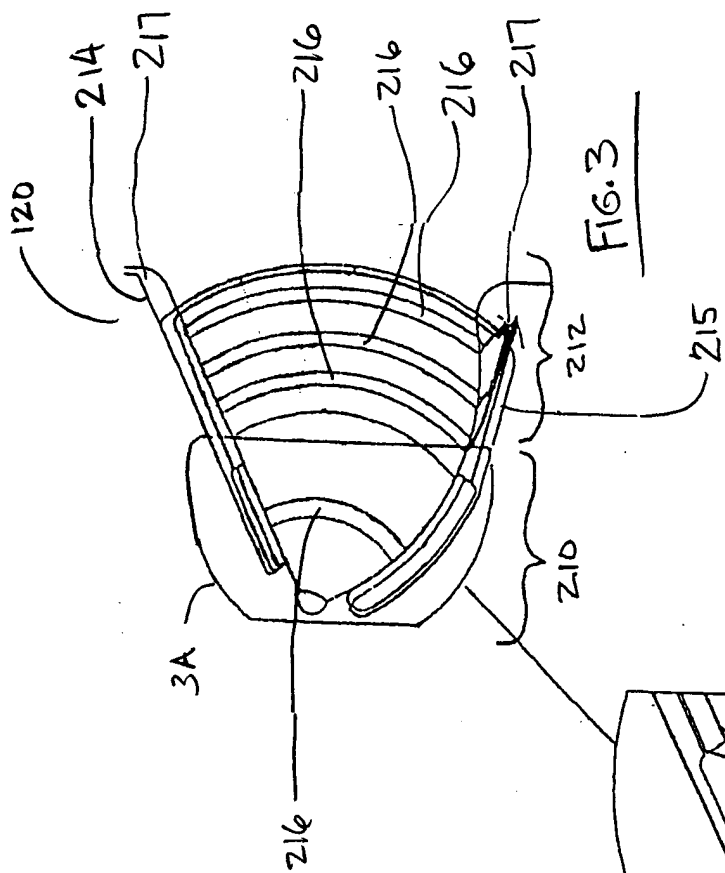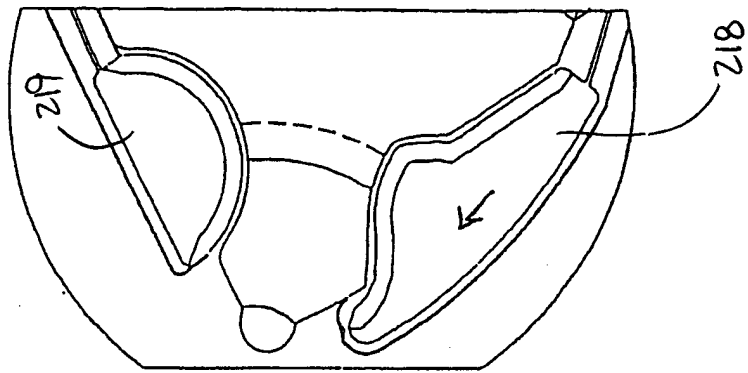

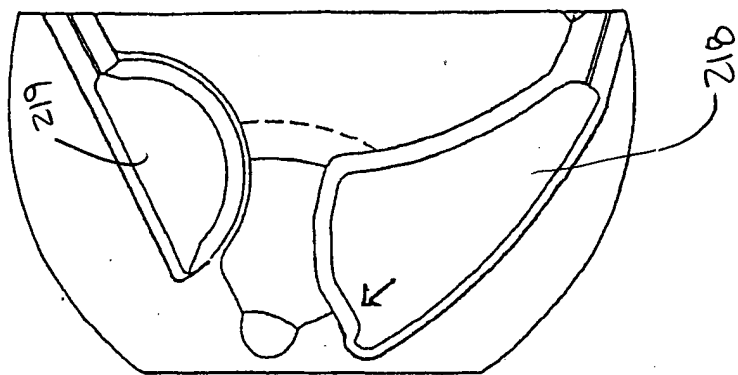

3B



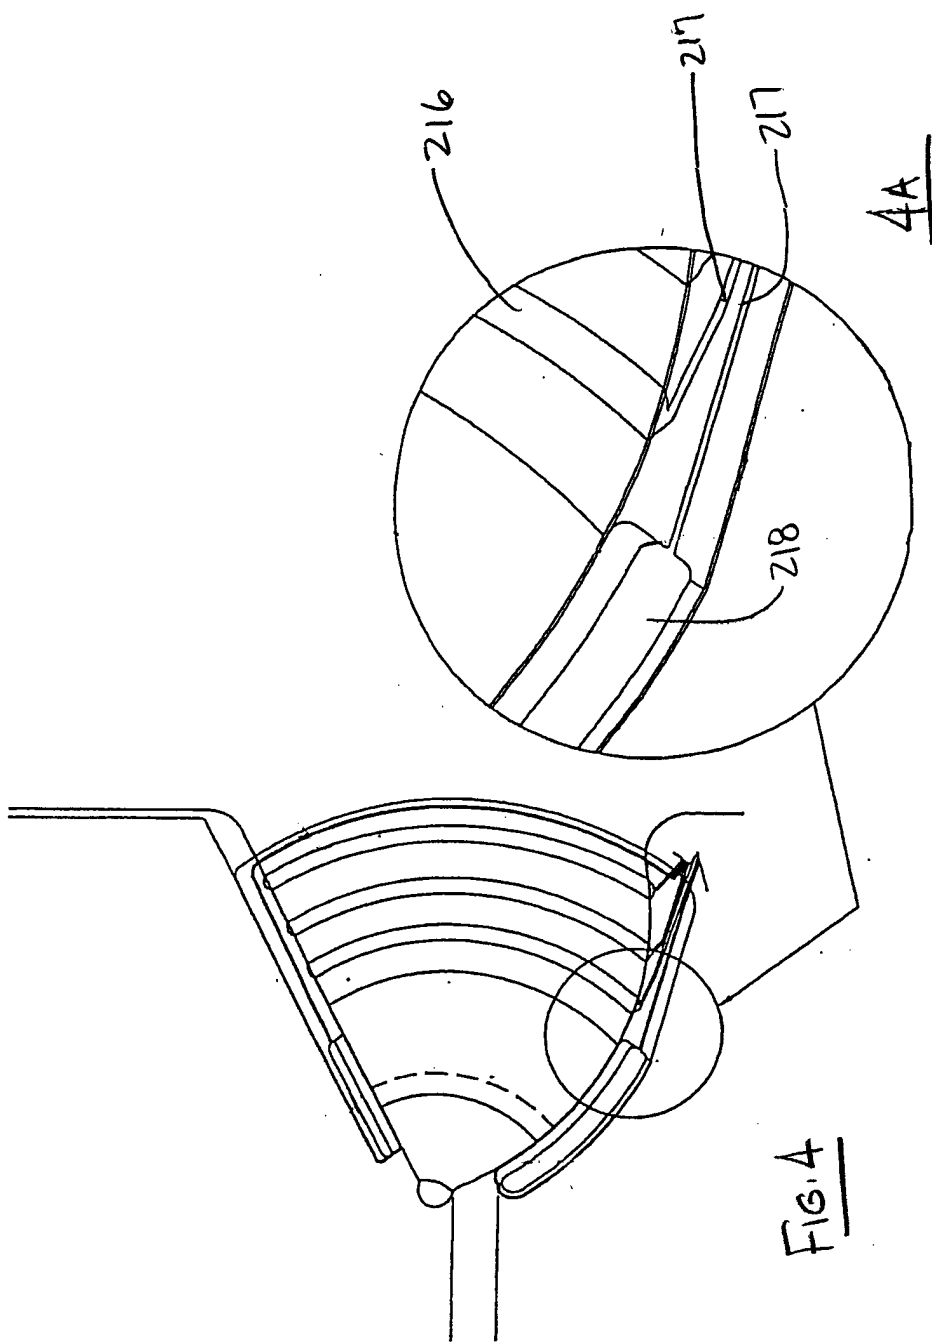

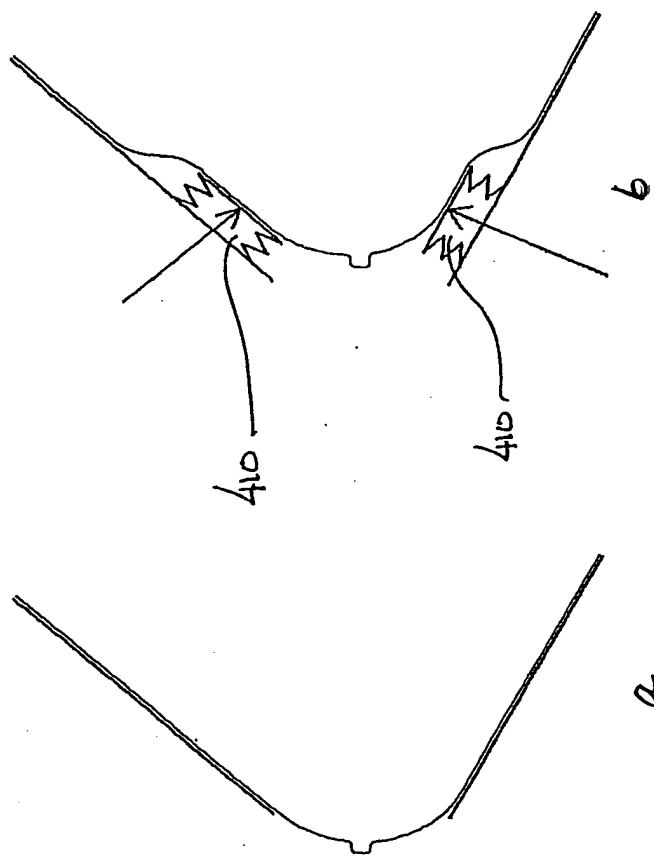


FIG. 5

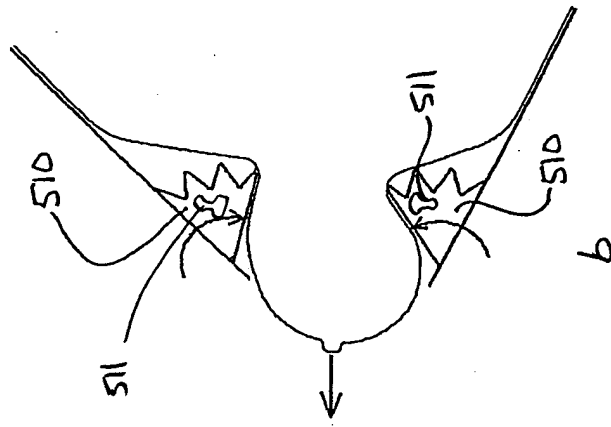
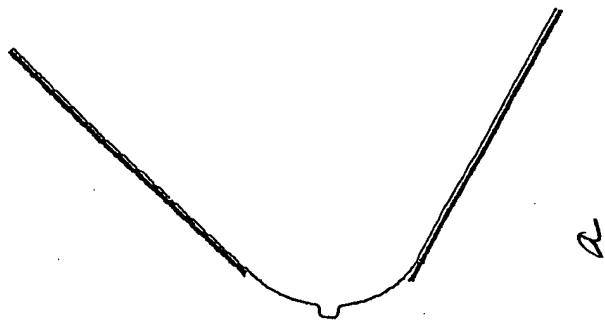


FIG. 6

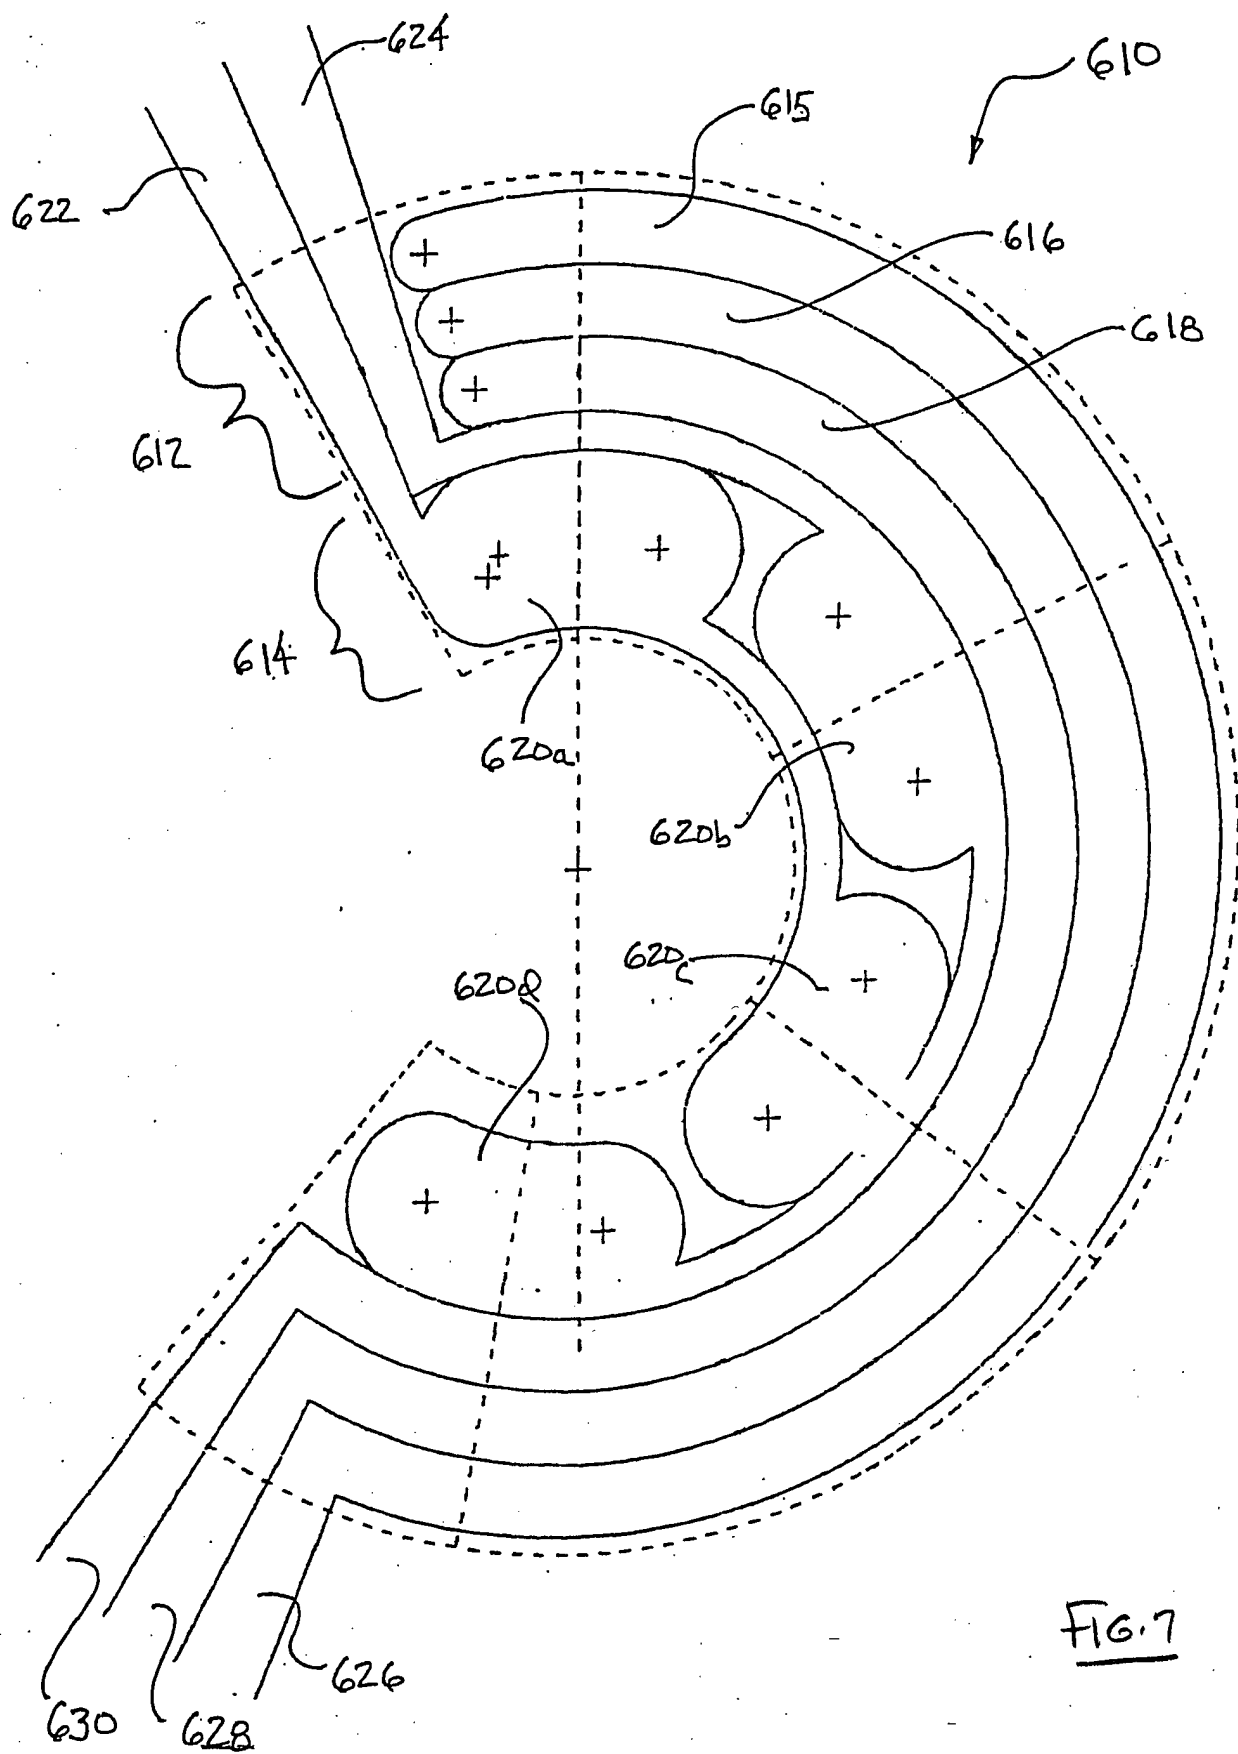


FIG. 7

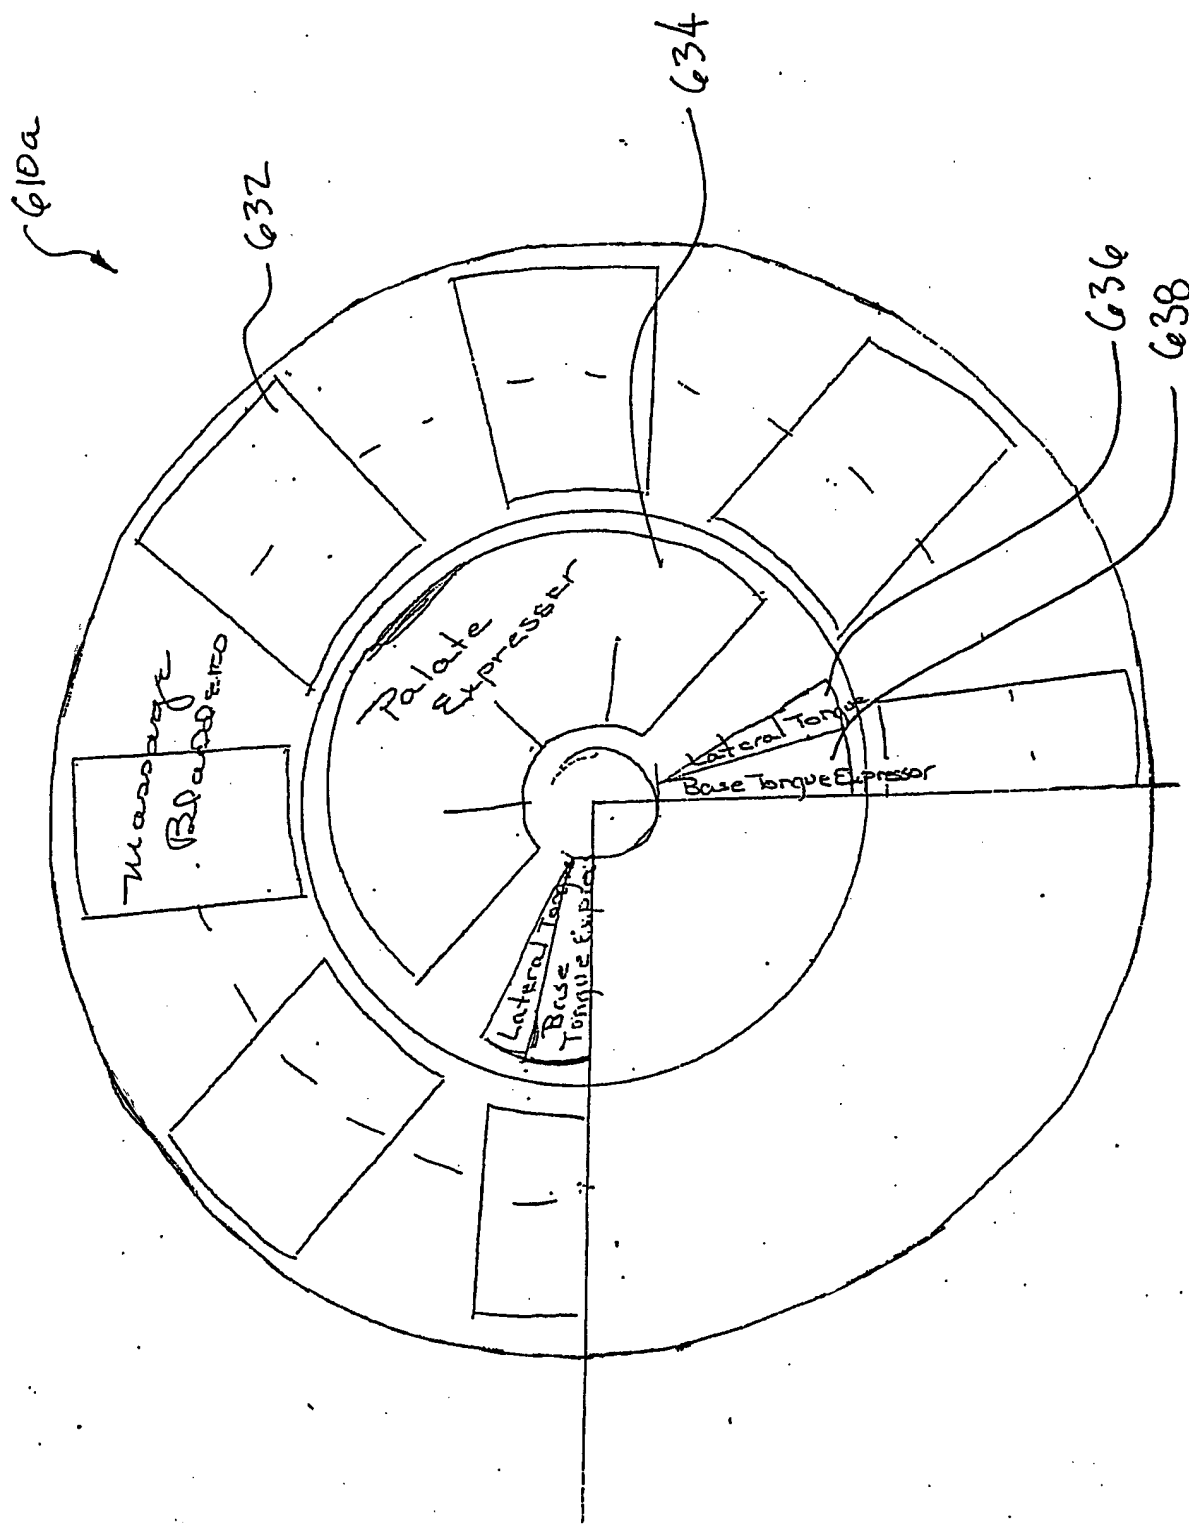


FIG. 8

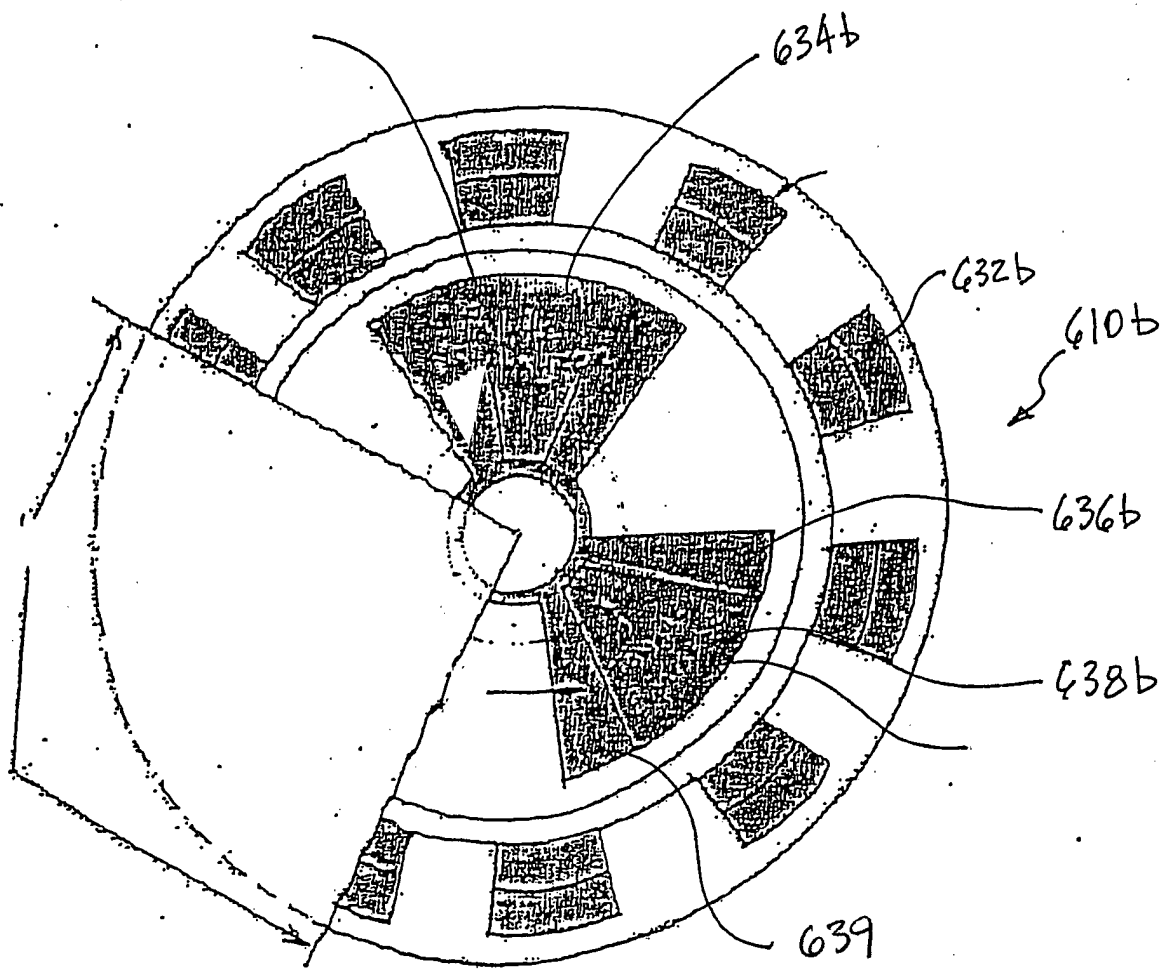


FIG. 9

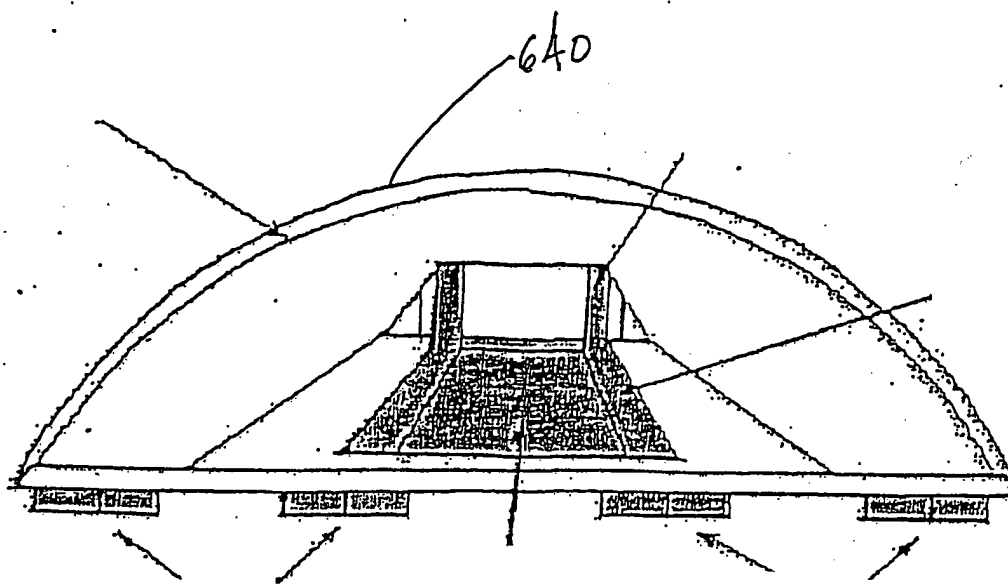


FIG. 10

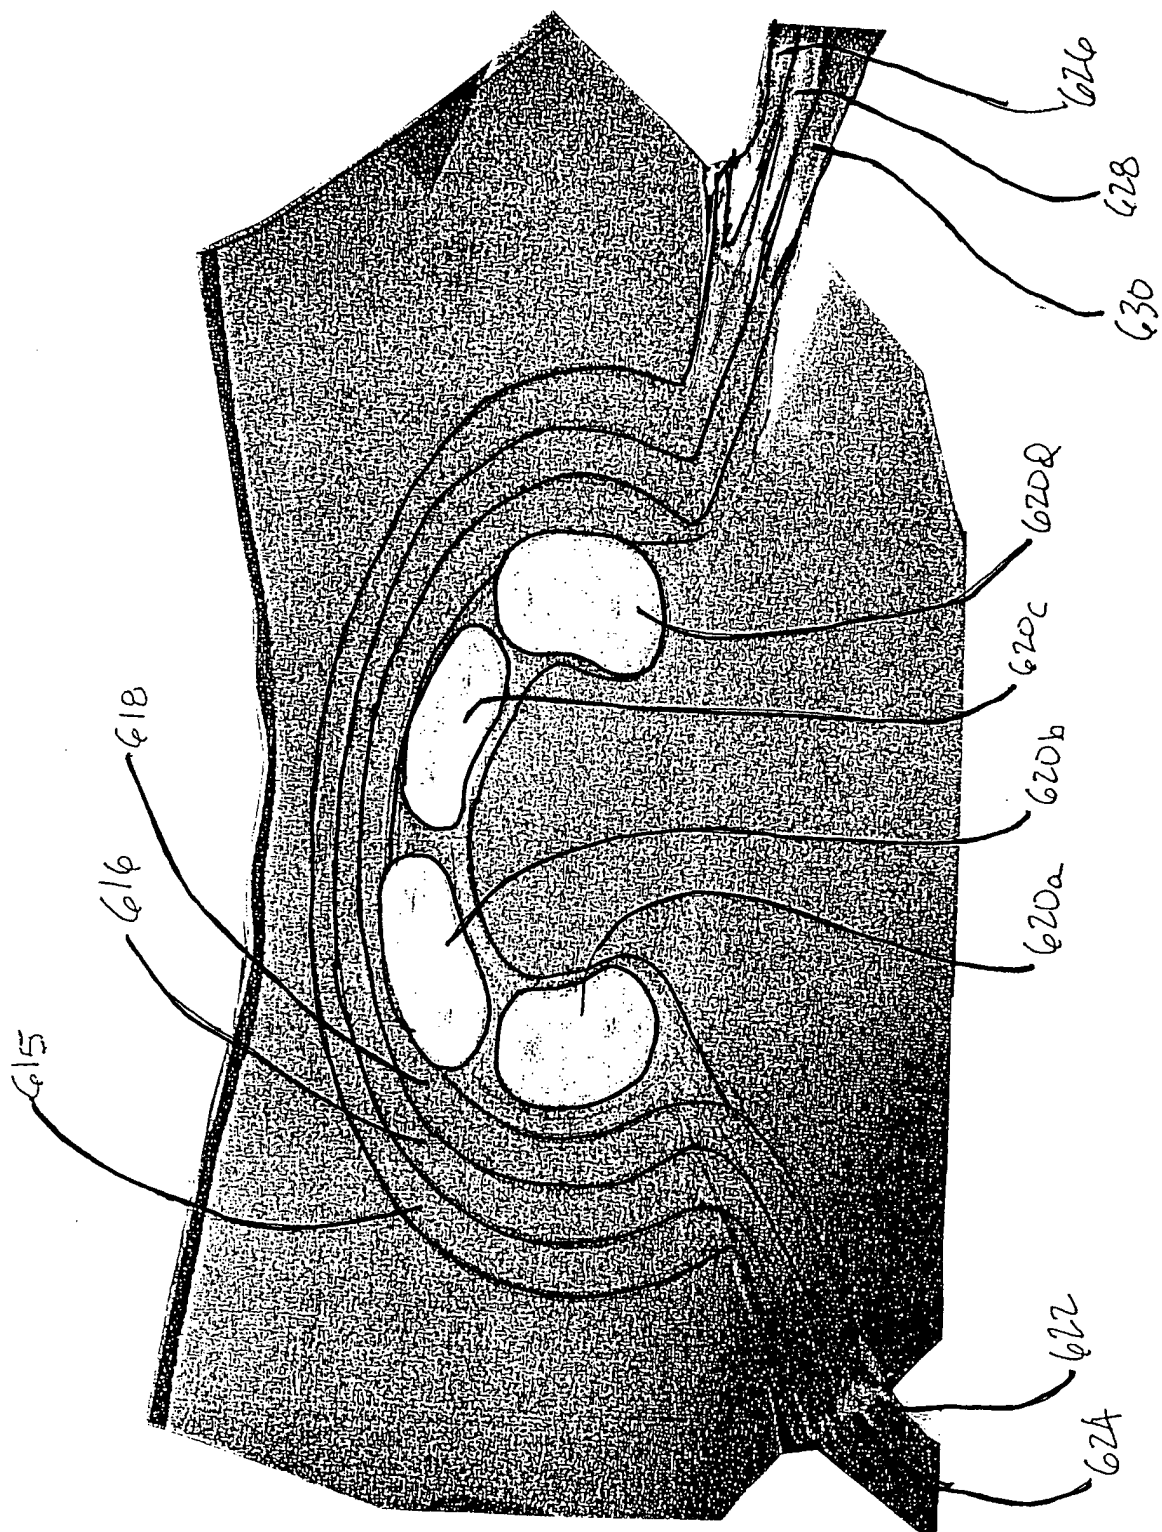


FIG. 11

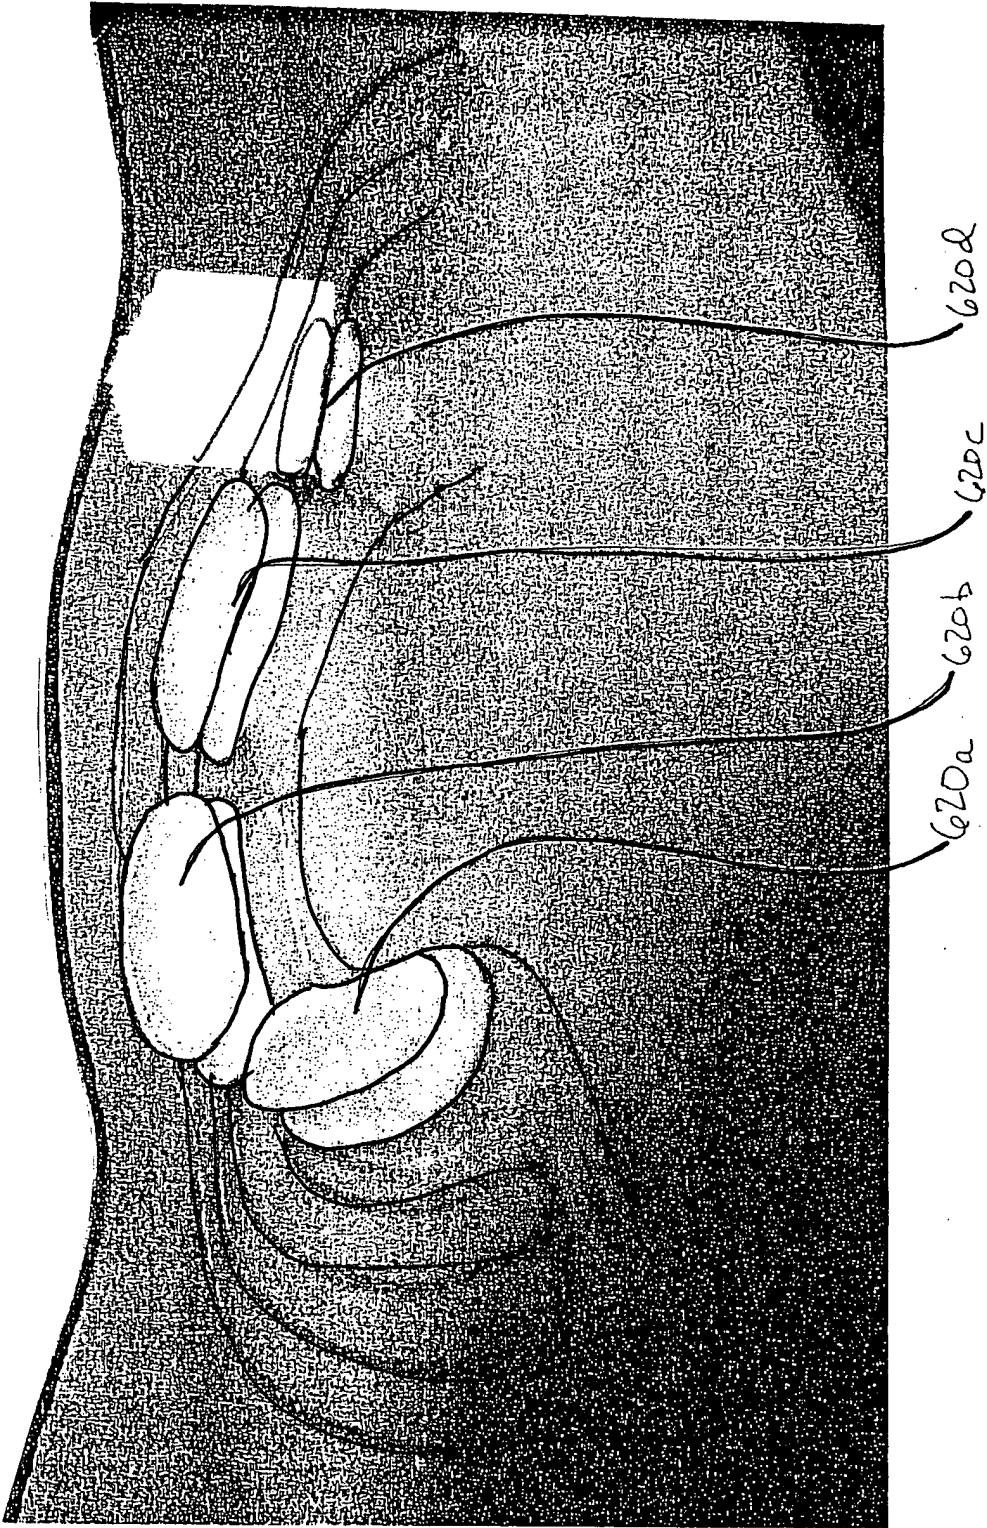


FIG. 12


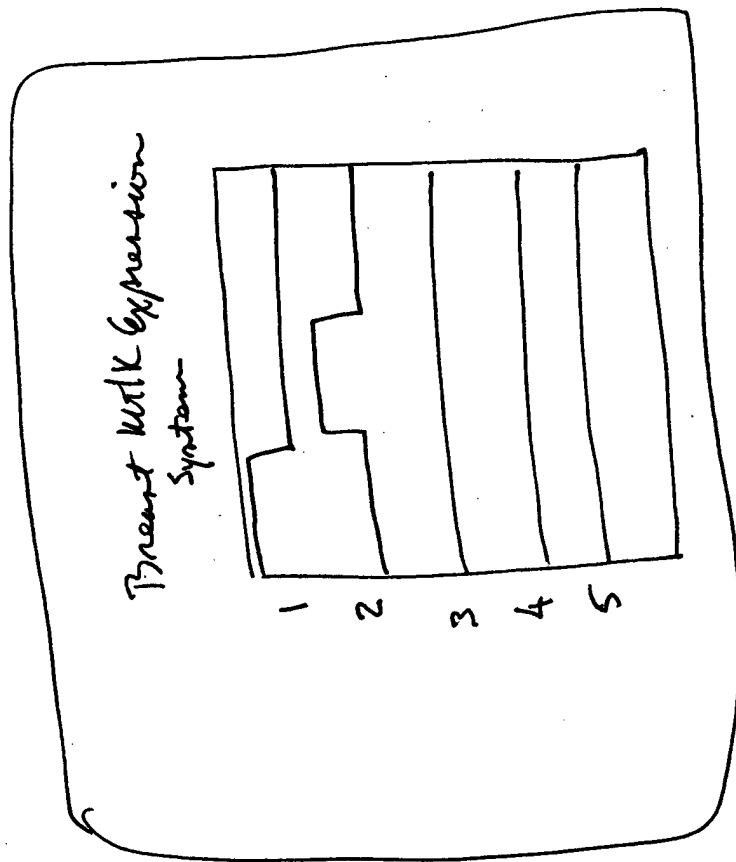


FIG. 13

Timing diagram for peristaltic bladder system inflation

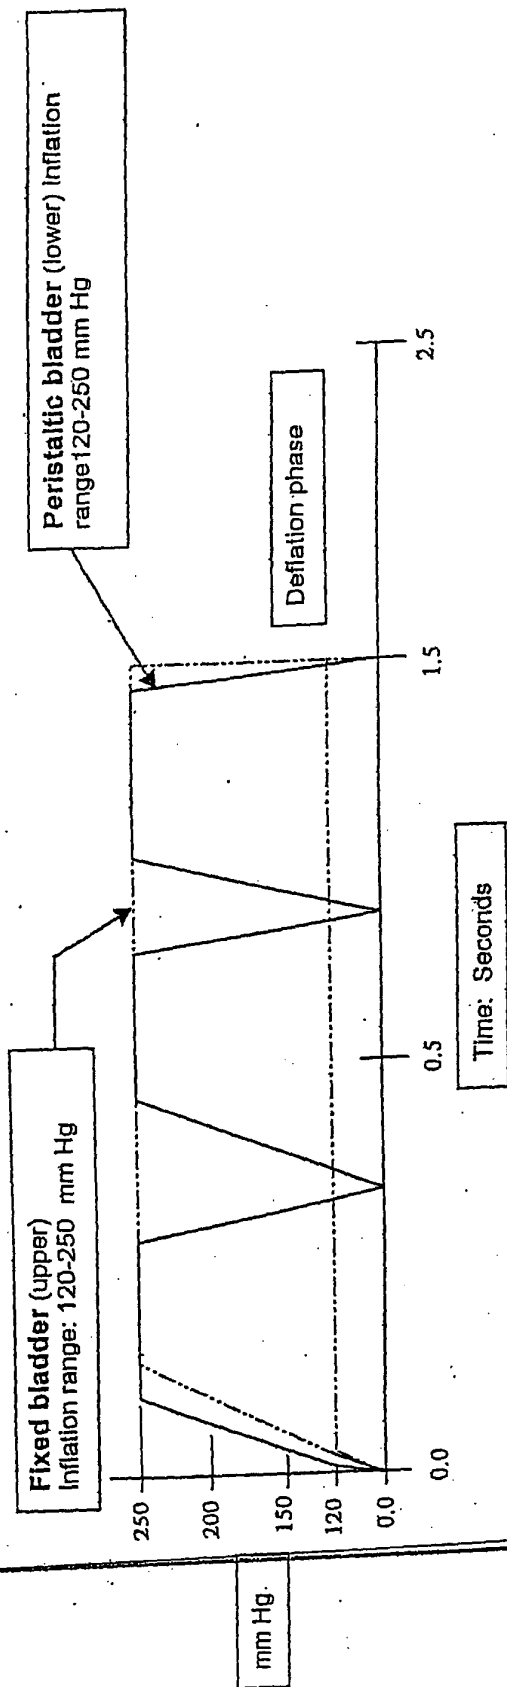

Timing diagram for ring bladder massage system inflation


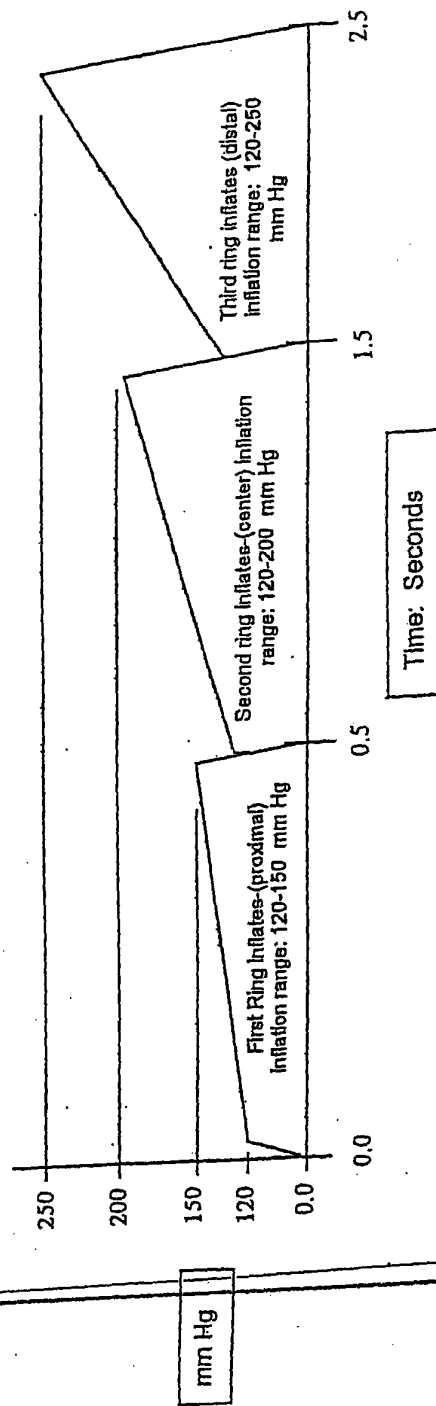


FIG. 14

The Ring bladder massage system must be controlled independently of the peristaltic/fixed bladder system

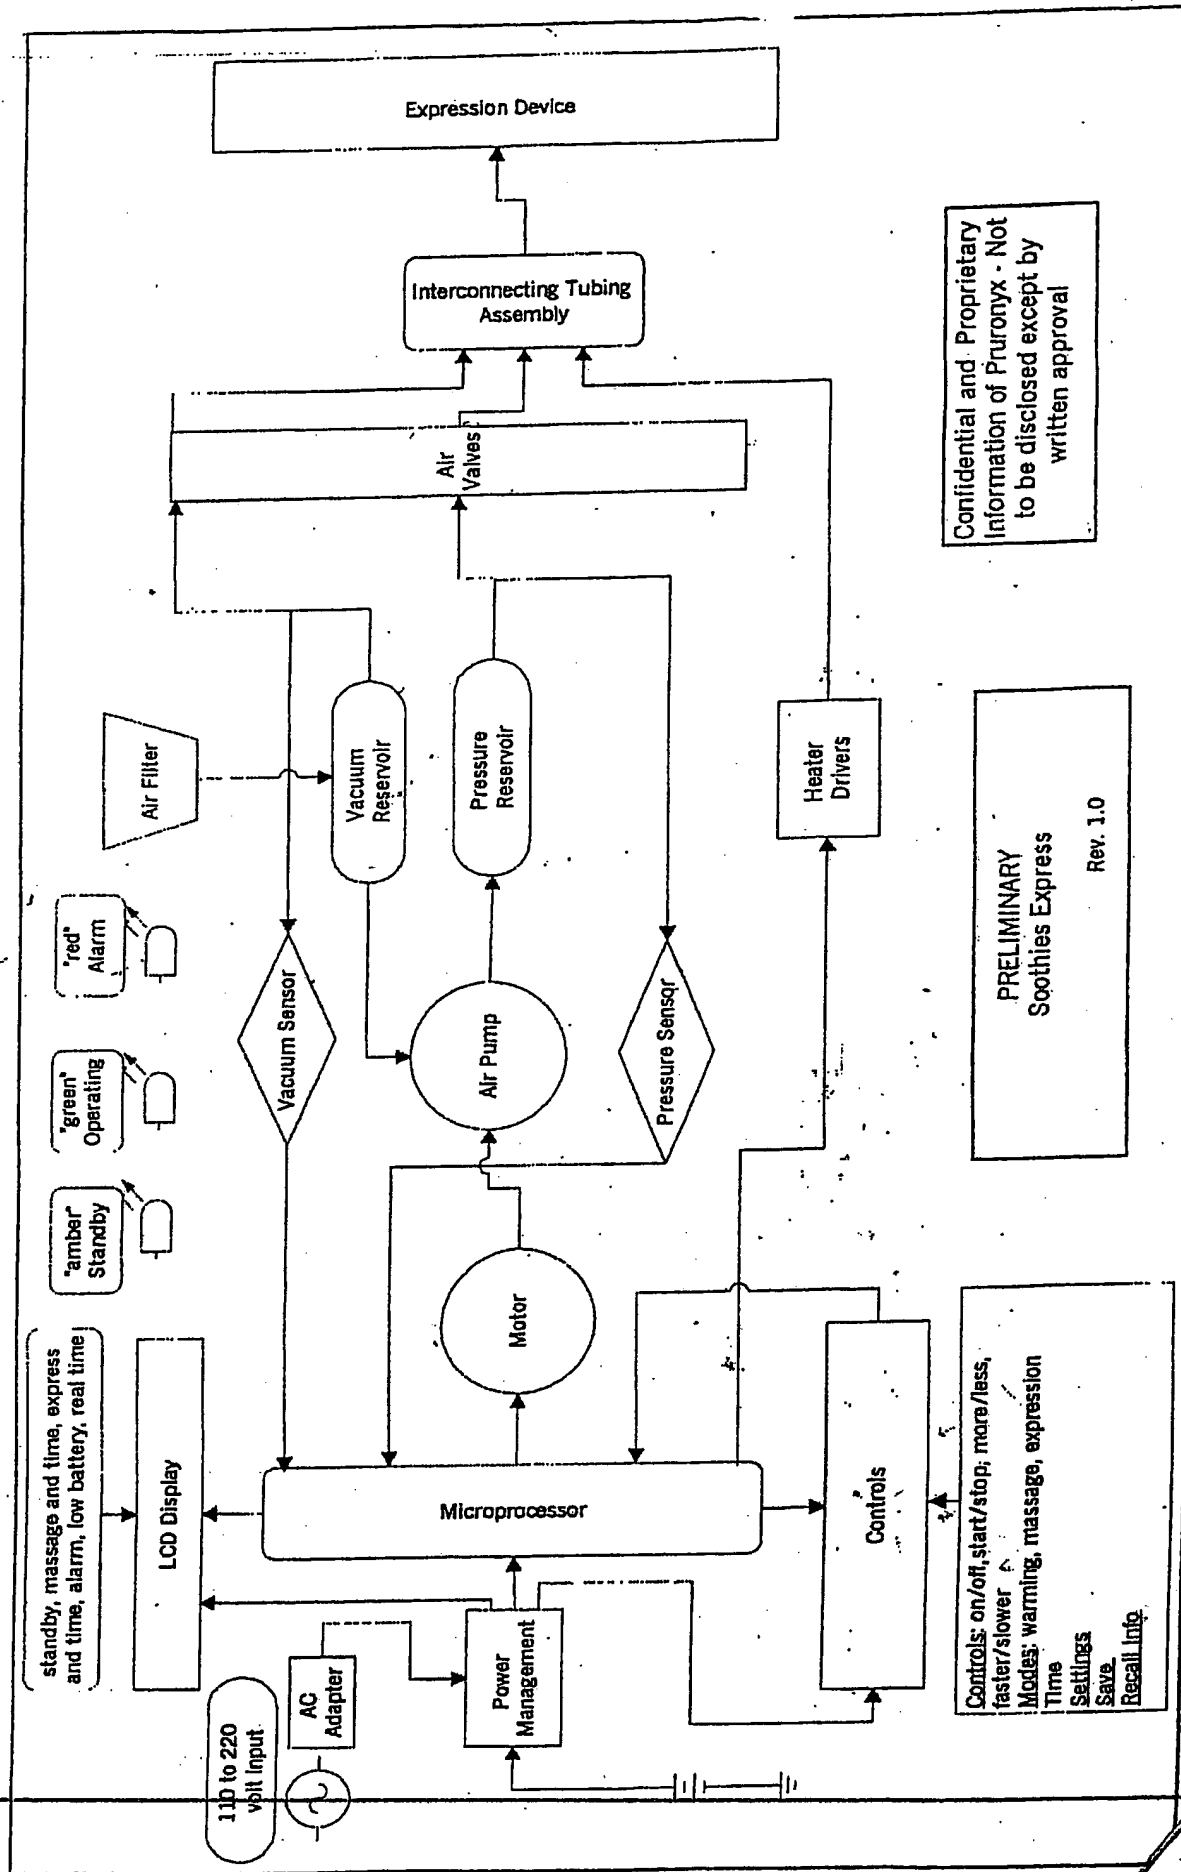

Confidential and Proprietary
Information of Prunonyx - Not
to be disclosed except by
written approval

PRELIMINARY
Soothies Express
Rev. 1.0

Controls: on/off, start/stop, more/less,
faster/slower
Modes: warming, massage, expression
Time
Settings
Save
Recall Info

FIG. 15